

COMPLETE OPTICAL QUALITY ANALYSIS OF A NON-LINEAR MICROSCOPE

Rodrigo Aviles-Espinosa¹, Rafael Porcar-Guezenc², Dobryna Zalvidea¹, David Artigas^{1,3},
Pablo Loza-Alvarez¹

¹ICFO-The Institute of Photonic Sciences, Mediterranean Technology Park, Av. Canal
Olimpic s/n, 08860 Castelldefels (Barcelona), Spain.

²Imagine Optic, 18 rue Charles de Gaulle, 91400 Orsay, France.

³Universitat Politècnica de Catalunya, c/ Jordi Girona 31, 08034 Barcelona, Spain

E-mail: rporcar@imagine-optic.com

KEY WORDS: Non-linear microscope, Two-Photon Excitation Fluorescence, Second Harmonic Generation, living cells, optical metrology, wavefront sensing, optical aberrations.

1. ABSTRACT

We investigate the optical quality of a custom made non-linear microscope and the associated sample aberrations through a systematic analysis based on wavefront sensing. Measurements are performed at each segment of the optical setup: before, inside, and after the non-linear microscope. Importantly, aberrations are also measured for the generated signal (fluorescence), in both, the forward and backward directions.

High resolution microscopy allows exceptional imaging quality and contrast resolving very small volumes thanks to the localized non-linear emission (TPEF, SHG or THG) [1]. Nevertheless, there are still several remaining limitations that cannot be overcome: the refractive indices mismatch caused by different materials and the sample itself, which both produce aberrations and lead to a reduction of image quality and contrast [2].

To overcome these problems, aberrations can be measured and corrected using adaptive optics. One of the easiest implementation in microscopy applications is the use of genetic algorithms to

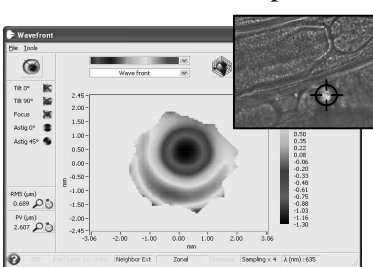


Figure 1: Residual wavefront map measured on TPEF signal from a living *C. elegans*. Inset shows the generated signal from inside the nematode.

control the adaptive component mainly because optimization can be performed on any measured signal relevant of image quality (intensity, focus, etc.) [3]. The drawback is the need of large amounts of iterations to reach the best correction, which usually produces phototoxic effects on the sample. We demonstrate that, in a non-linear microscope, it is possible to reduce the number of iterations using a Shack-Hartmann wavefront sensor. This is done by taking a single measurement of the generated TPEF beam from the sample plane (see figure 1). This greatly reduces the biological sample exposure. If combined with adaptive optics, this technique could open the door to living high resolution observation, in real time, with increased penetration depths in the sample.

2. ACKNOWLEDGMENTS

The research leading to these results has received funding from the European Community's under grant agreement FP7-PEOPLE-2007-3-1-IAPP -217997. This work has been partially funded by Fundació Cellex. DZ wants to acknowledge to MICINN through Ramon y Cajal program.

3. REFERENCES

- [1] Chris Xu Et al., “Multiphoton fluorescence excitation: new spectral windows for biological nonlinear microscopy”, *Proc. Nat. Acad. Sci. USA* 10763-10768 (1996/10).
- [2] Martin Booth, “Adaptive optics in microscopy”, *Phil. Trans. R. Soc. A* 2829–2843 (2007/09).
- [3] A. J. D. Wright Et al. “Optimization Algorithms for the implementation of adaptive optics in confocal and multiphoton microscopy”, *Microscop. Res. Tech* (2005 /67).